



Fridge-tag® 2|2E

User Guide

Table of Contents

Overview	4
Fridge-tag 2.....	4
Fridge-tag 2 E.....	4
The Extended Solution.....	4
Display Explanations.....	6
State of Delivery / Sleep Mode.....	7
Placing the Fridge-Tag.....	9
Activation Process.....	10
Overview	10
Device Activation	11
Setting the Calendar Format.....	11
Using the READ and the SET buttons	12
Setting the Date	13
Setting the Time.....	15
Setting the Alarm Limits (if preset by factory).....	17
LOC function (internal sensor only).....	21
Connection error (external sensor only).....	22
Read and Change Settings.....	23
Overview: menu.....	23
Initial menu (read and change settings)	24
Screen Displays During Measurement Mode.....	26
Example OK display – during measurement	26
Example Alarm Display – During Measurement.....	26

Alarm Trigger Function.....28

Alarm Display and Confirmation options..... 29

Cumulative Daily Time Above/Below the Limit 32

Reading History / Readout Mode34

Option 1: Read From Device (30-Day History)..... 34

Option 2: Read Alarms on the Device (Alarm Super Jump Function)..... 37

Option 3: Read Data from the Files Generated by the Fridge-Tag..... 38

PDF Report Explanation..... 40

Temperature Record Duration (Optional Factory Setting) 41

Verification process..... 42

Explanations of terms.....44

Expire code explanation 44

Important Information.....45

Liability..... 45

Battery 45

Useful life 45

Attention..... 46

Regulatory certification 46


FAQ / Glossary.....47

Frequently Asked Questions (FAQ) 47

Glossary of Symbols 47

Overview

This section provides an overview of Fridge-tag 2 and Fridge-tag 2E monitors.

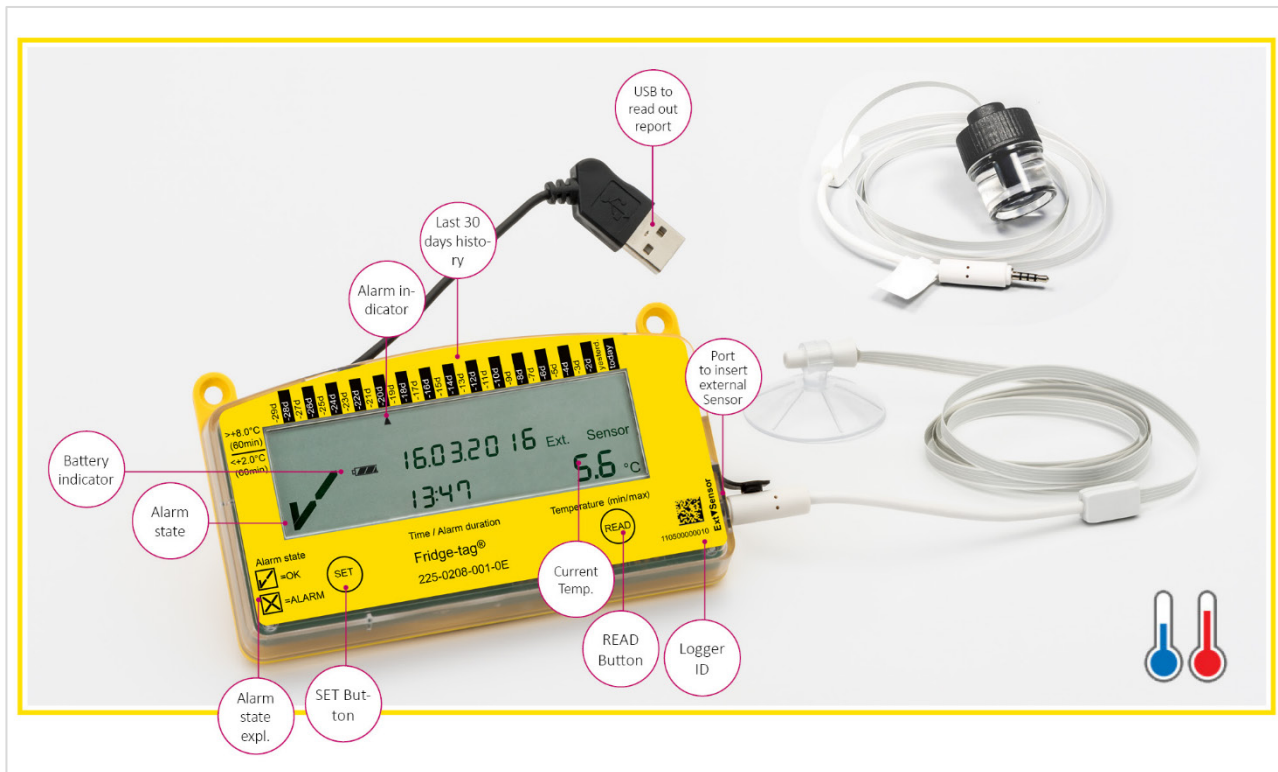

Fridge-tag 2

The Intelligent Solution

The Fridge-tag 2 measures the ambient temperature every minute and immediately issues an alert when your alarm limit is exceeded.

- Robust housing design
- Easily readable display

WHO PQS E006/020

Fridge-tag 2 E

The Extended Solution


The Fridge-tag 2 E measures the ambient temperature every minute and immediately issues an alert when your alarm limit is exceeded.

- Extended lifetime up to 5 years
- Robust housing design

- Easily readable display

WHO PQS E006/040

Display Explanations

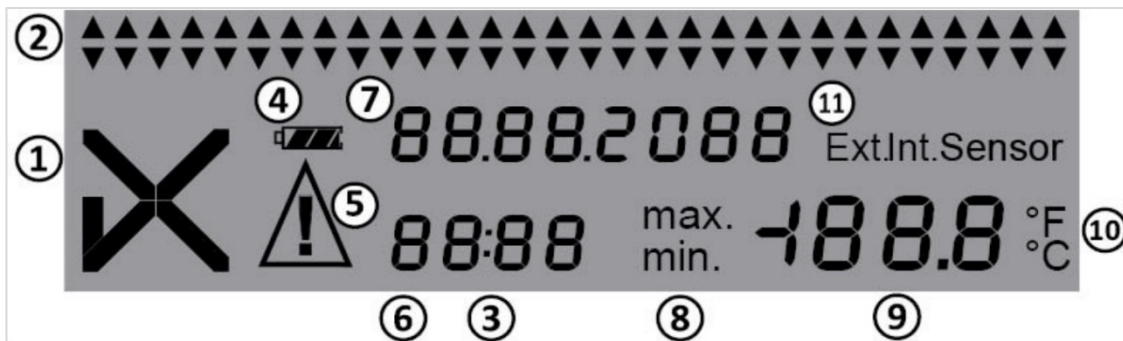


1. ✓ (OK symbol) or ✕ (alarm symbol)
 2. Daily HIGH/LOW alarm indicators ▲ ▼ (showing the history of the last 30 days)
 3. Power indicator (colon is flashing)
 4. Battery indicator (indicates the remaining capacity of the battery)
 5. Additional warning symbol ⚠
 6. Time, duration and text display
 7. Date and text display
 8. Display of measured minimum/maximum temperature
 9. Temperature display
 10. Display of the temperature measurement unit (°F/°C)
 11. Display of the activated sensor: Int. = internal sensor
- Ext. = external sensor (cable with temperature sensor)

Note: All illustrations in the User Manual refer to the Fridge-tag with internal sensor. Differences between internal and external sensors are additionally described.

State of Delivery / Sleep Mode

The Fridge-tag is shipped in sleep mode.

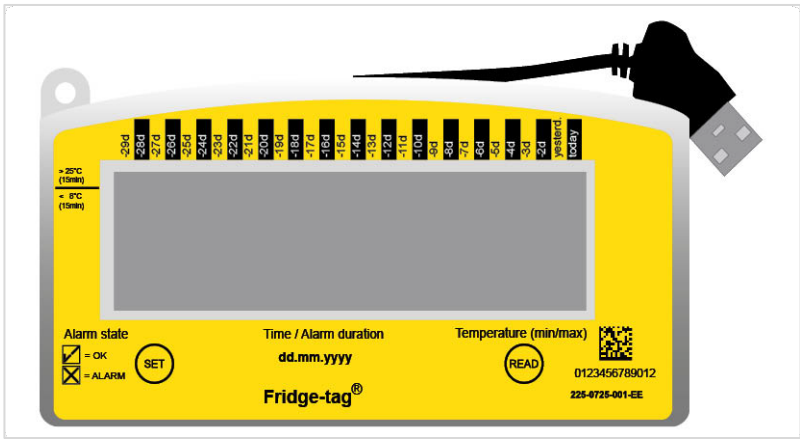


The display (LCD) is blank.

Read out information prior to activation (in sleep mode)







The following page shows which information will be indicated on the screen upon successive READ button pressings while in sleep mode.

Note: After approx. 60 seconds without pressing any button on the Fridge-tag the devices goes back into sleep mode; the display is blank again.

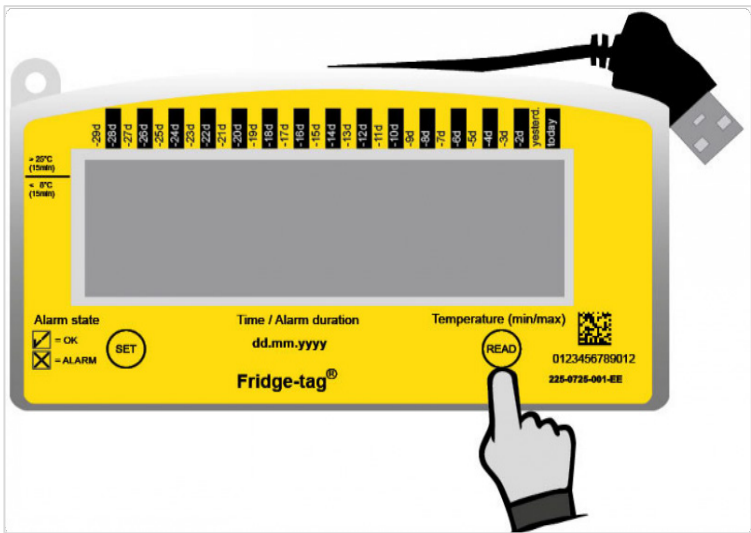

Press repeatedly **READ** to gather information.

After 1st pressing of READ		Display test: all segments activated
----------------------------	---	---

After 2nd pressing of READ		Indication of date and production test result: 16 February 2018/PASS (quality check passed)
After 3rd pressing of READ		Indication of the current temperature and which sensor is activated (internal/external). Display shows —.°C if external sensor is not connected.
After 4th pressing of READ		Indication of configuration ID (e.g. 1234)
After 5th pressing of READ		Indication of upper alarm settings. Example shows duration and temperature limits: 10 hours, >+8°C, high
After 6th pressing of READ		Indication of lower alarm settings. Example shows duration and temperature limits: 1 hour, <-0.5°C, low
After 7th pressing of READ		Serial number of the device
After 8th pressing of READ		PCb number (manufacturer information)
After 9th pressing of READ		Battery power: 3 bars = full (>70%) 2 bars = half-full (>30–70%) 1 bar = low (0–30%)** **Device should be replaced.
After 10th pressing of READ		Disable user clock adjust. For more information, please see Activation Process section.
After 11th pressing of READ		The display is blank again.

Placing the Fridge-Tag

This section describes how to place a fridge-tag with an internal and external sensor.

With an Internal Sensor

The activated Fridge-tag must be placed immediately after activation in its predetermined location. It is recommended and important to place the device in the center of the refrigerator for an optimal temperature observation.

Please do not place the device into a freezer as the screen will freeze and the battery will lose power prematurely.

With an External Sensor

Two hours before activating the Fridge-tag the external sensor must be placed in its predetermined location. It is recommended and important to place the external sensor in the center of the refrigerator for an optimal temperature observation and to avoid any incorrect measurements when starting the device.

For the right positioning of the external sensor within the fridge, please follow the instructions of WHO, CDC or any other governmental requirements of your country.




- External Sensor
- Flat cable
- Fridge-tag

Activation Process

This section describes activation process.

Overview

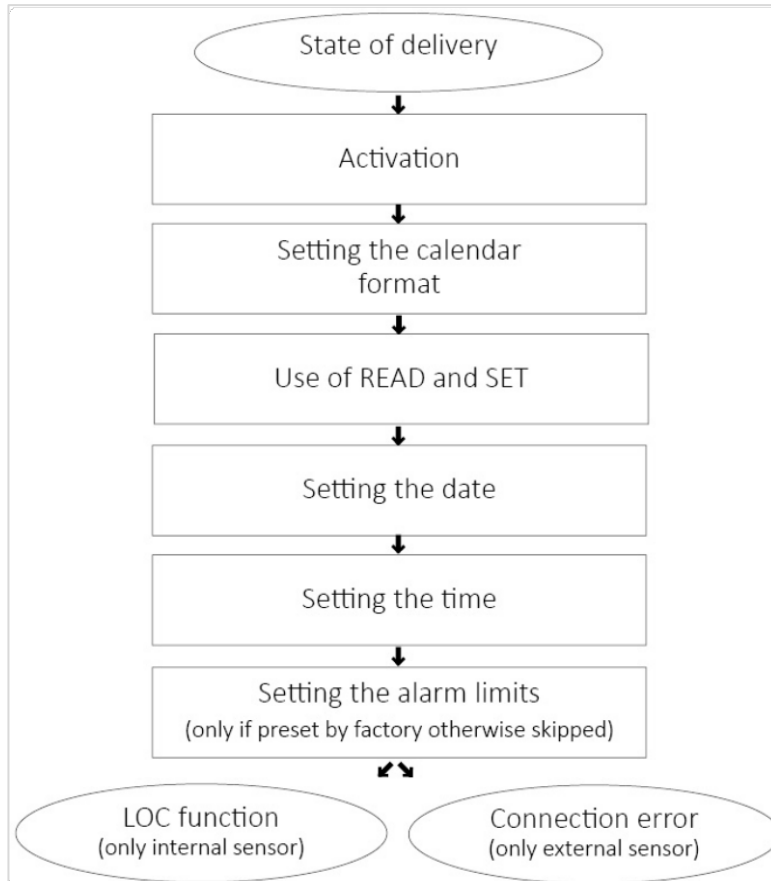


Note: As long as the activation process has not been completed, after approx. 60 seconds without any button operation, the device will go back into sleep mode. The activation has to start from the beginning.

If you want to read or change settings (e.g. change °F to °C) after the activation has been completed, proceed as described in the [Read and Change Settings](#) section.

Device Activation

To activate the device press, the **SET** and the **READ** button simultaneously during at least 3 seconds:

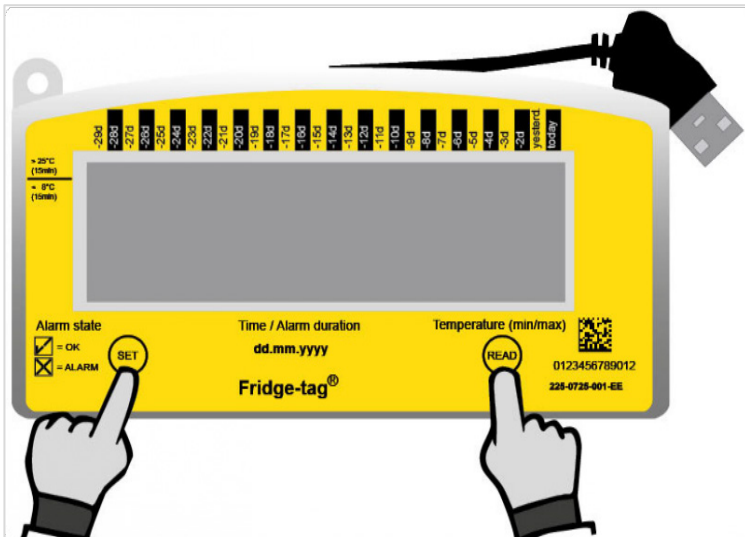


Note: Once the device is activated, it cannot be stopped anymore.

Activation has been successful when the following indication appears on the screen:




Setting the Calendar Format

Option 1: dd.mm.yyyy Format

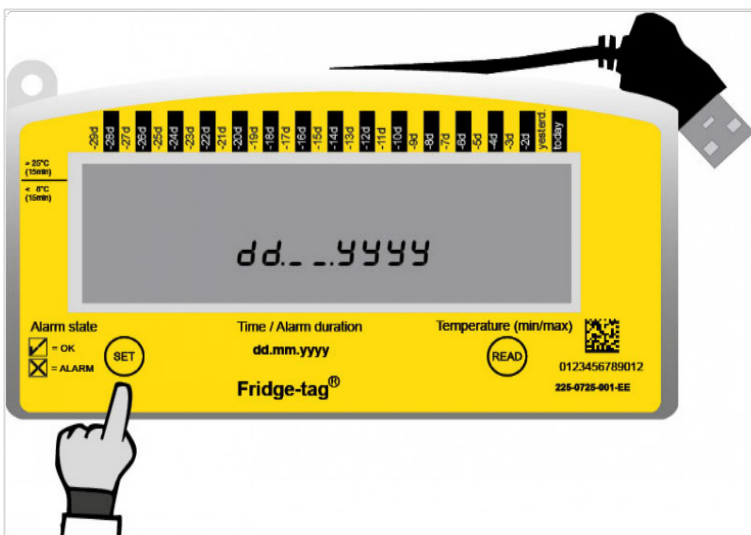

Press **SET** to save the calendar format.

Option 2: mm.dd.yyyy Format

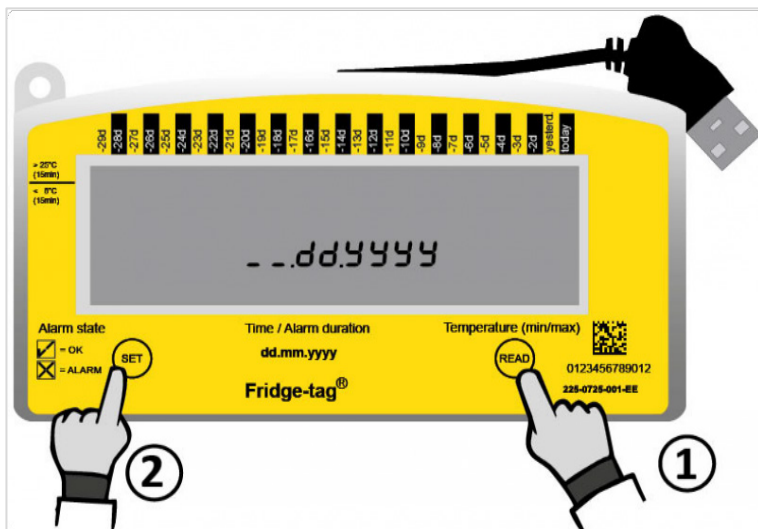


1. Press **READ** to change the calendar format.
2. Then press **SET** to save the calendar format.

After setting the calendar format, the first digit of the date will start flashing.

Using the READ and the SET buttons

READ button

The **READ** button is used to adjust the numbers. Each time you press the **READ** button, the number in the flashing digit will increase by 1. If you press **READ** more than necessary, continue pressing the **READ** button until you obtain the desired number.

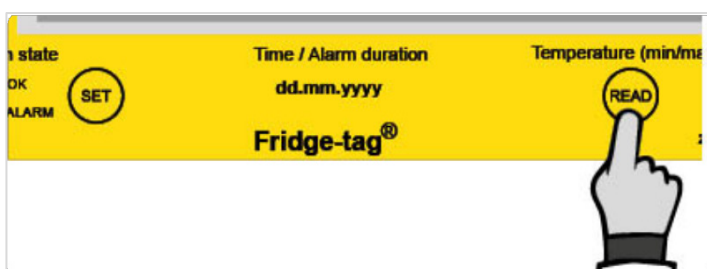

Press **READ** to adjust the number

SET button

The **SET** button is used to save the number. After pressing the **SET** button, the next digit will start flashing.




Press **SET** to confirm.

Note: If **SET** is pressed mistakenly, continue with the setup instructions. The [Read and Change Settings](#) section describes how to rectify the error.

Setting the Date


The following example shows how to set the date to: 16 February 2018 (16.02.2018) in European format.

The 1st digit is flashing.

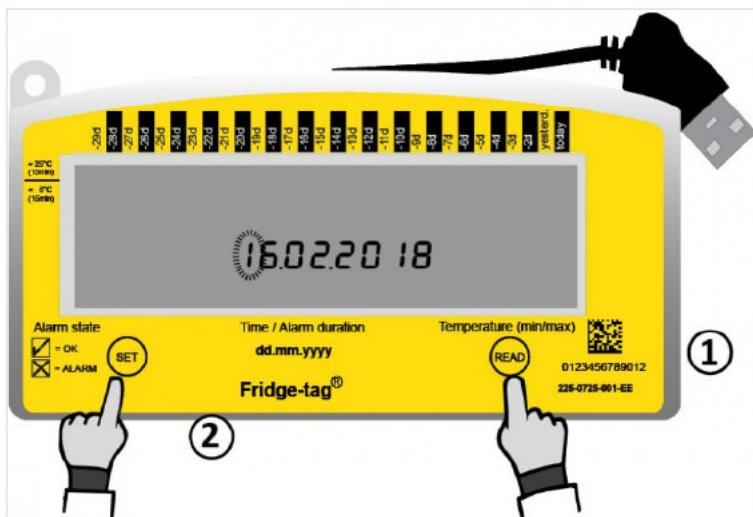


Press **READ** until "1" appears as the first digit.
Press **SET** to save.

The 2nd digit is flashing.

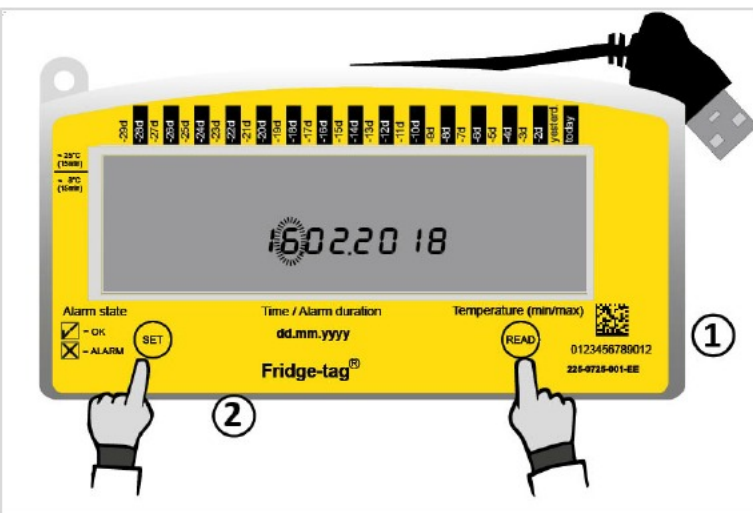


Press **READ** until "6" appears as the second digit.
Press **SET** to save.

The 3rd digit is flashing.

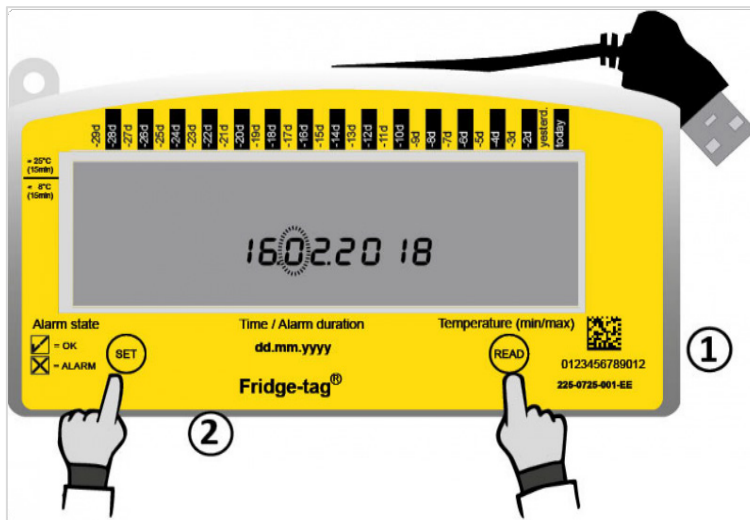

Press **READ** until "0" appears as the third digit.
Press **SET** to save.


The 4th digit is flashing.

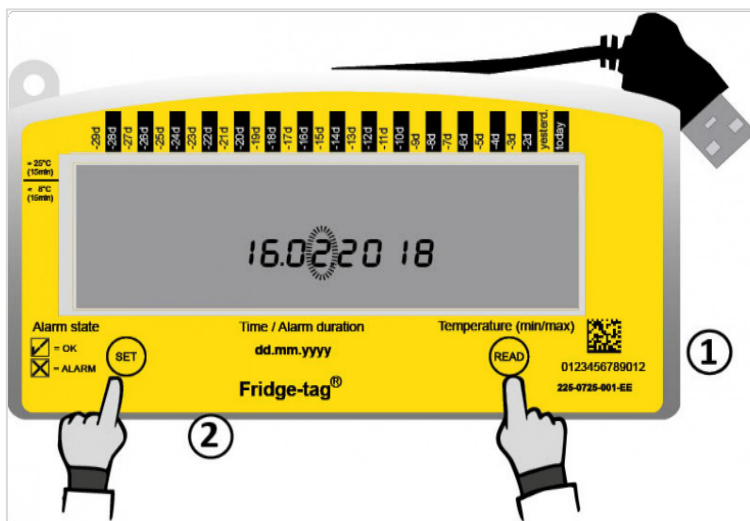

Press **READ** until "2" appears as the fourth digit.
Press **SET** to save.


Note: The fifth and the sixth digit are set automatically.

The 7th digit is flashing.

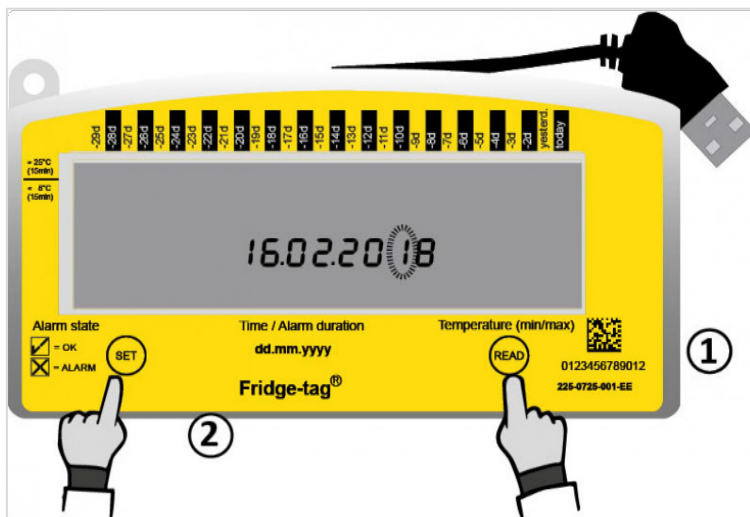

Press **READ** until "1" appears as the seventh digit.
Press **SET** to save.

The 8th digit is flashing.

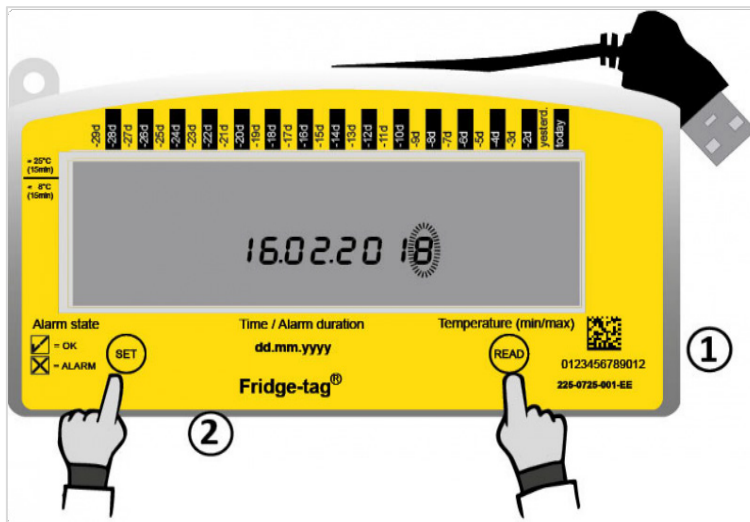

Press **READ** until "8" appears as the eighth digit.
Press **SET** to save.

The date is now set to: 16.02.2018.


Note: After setting the date, the first digit of the time will start flashing.

Setting the Time

This example shows how to set the time to 13:47.


Note: The clock operates a 24-hour clock (e.g. 1:47 pm = 13:47).

The 1st digit is flashing:

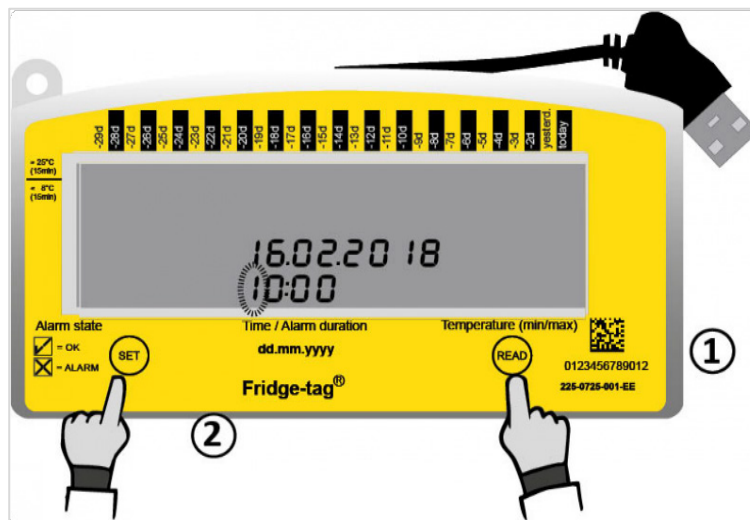


- Press **READ** until "1" appears as the first digit.
- Press **SET** to save.

The 2nd digit is flashing.

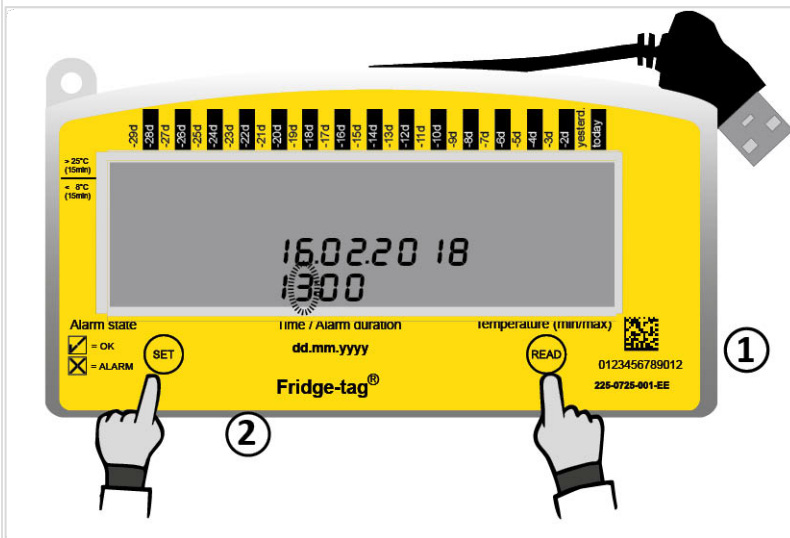


- Press **READ** until "3" appears as the second digit.
- Press **SET** to save.

The 3rd digit is flashing.

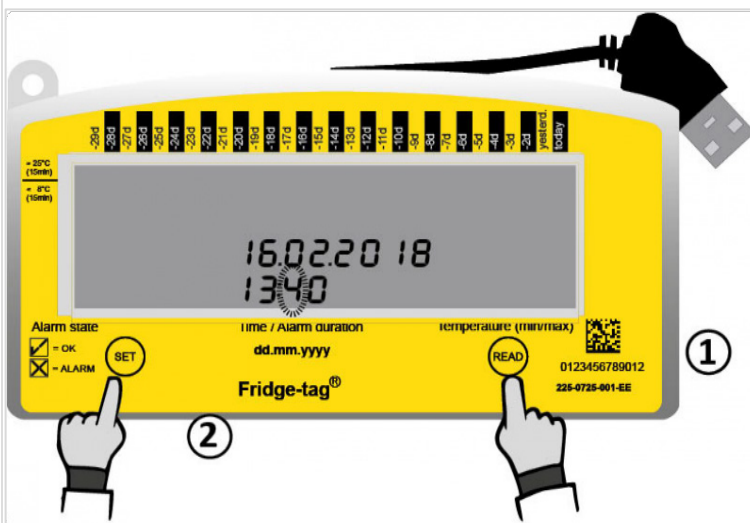

- Press **READ** until "4" appears as the third digit.
- Press **SET** to save.

The 4th digit is flashing.

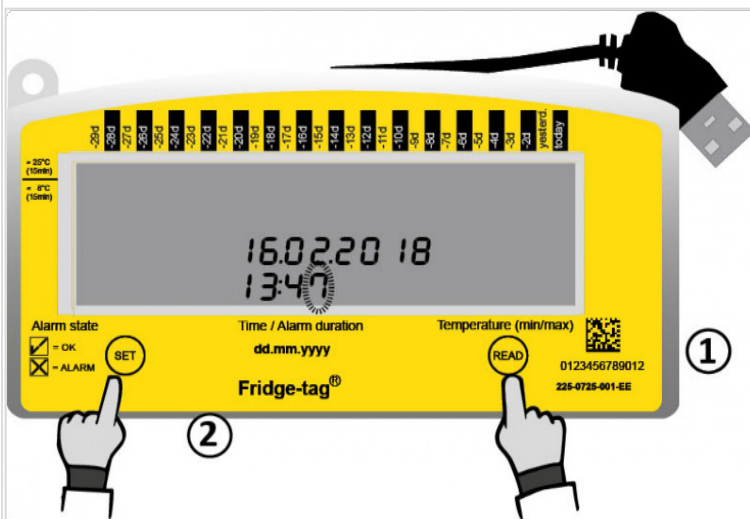

- Press **READ** until "7" appears as the fourth digit.
- Press **SET** to save.

The time is now set to 13:47.

Note: If the device is configured with self-programmable alarm limits proceed with the following the instructions in the [Setting the Alarm Limits \(if preset by factory\)](#) section.

As soon as the last digit of the time setting is confirmed, the activation is completed.

Internal sensor: Now place the Fridge-tag according to the [Placing the Fridge-Tag](#) section.

External sensor: Connect the device with the external sensor. During max. 1 minute after activation no temperature is displayed on the screen.


Setting the Alarm Limits (if preset by factory)

This adjustment is done in 4 steps:

1. Setting the duration of the upper alarm limit
2. Setting the temperature of the upper alarm limit
3. Setting the duration to the lower alarm limit
4. Setting the temperature of the lower alarm limit


Steps 1 and 3, and steps 2 and 4 are completed in the same manner, respectively

The 1st digit of the duration of the alarm limit is flashing.

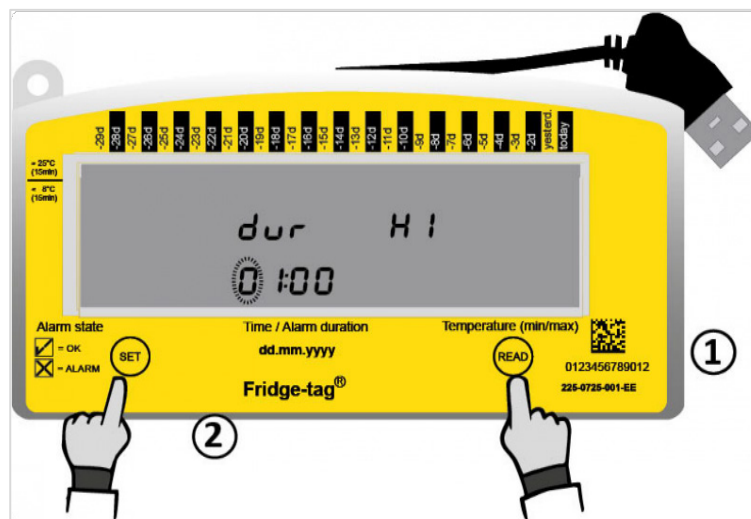


- Press **READ** to adjust the number.
- Press **SET** to confirm the number.

The 2nd digit of the duration of the alarm limit is flashing.

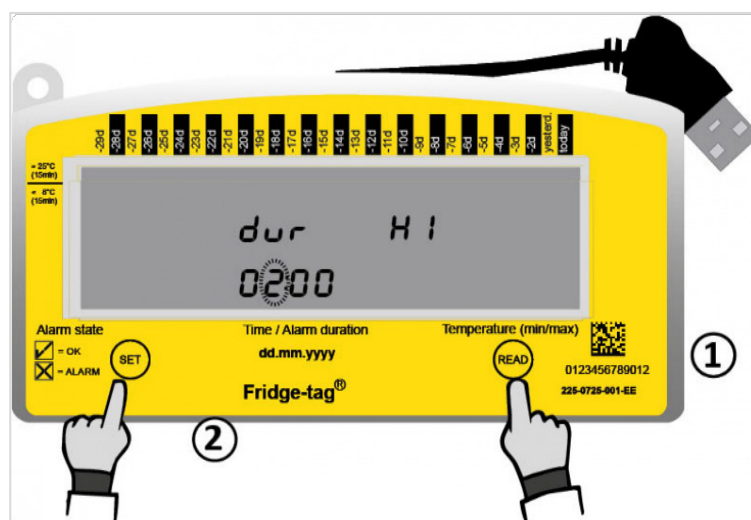


- Press **READ** to adjust the number.
- Press **SET** to confirm the number.

The 3rd digit of the duration of the alarm limit is flashing.

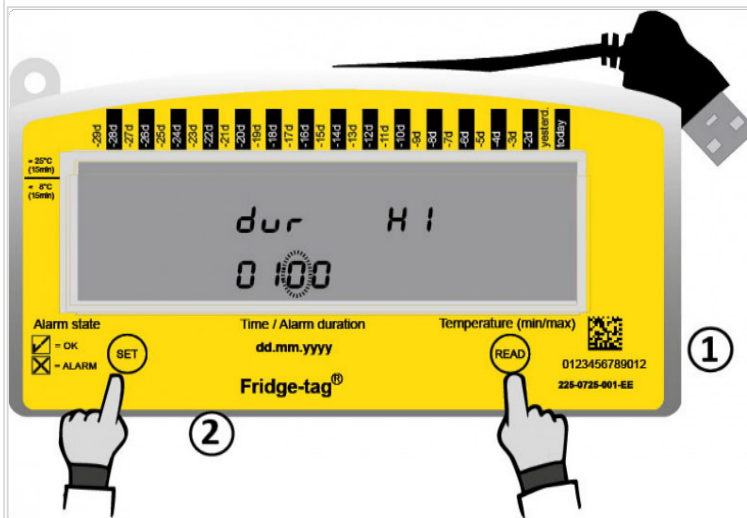

- Press **READ** to adjust the number.
- Press **SET** to confirm the number.

The 4th digit of the duration of the alarm limit is flashing.

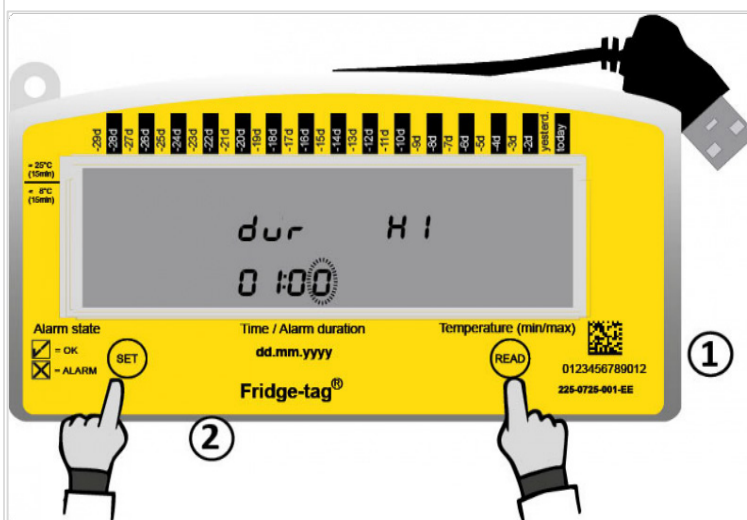

- Press **READ** to adjust the number.
- Press **SET** to confirm the number.


The duration of the alarm limit is now set.

- **Internal sensor:** Alarm temperature limits must be no lower than -20°C (-4°F) and no higher than $+50^{\circ}\text{C}$ ($+122^{\circ}\text{F}$).
- **External sensor:** Alarm temperature limits must be no lower than -35°C (-31°F) and no higher than $+55^{\circ}\text{C}$ ($+131^{\circ}\text{F}$).

First you have to choose the range of the desired temperature limit. You have the choice between negative and positive temperatures. In case of a positive limit in Fahrenheit you may further choose if the limit shall be equal or above $+100^{\circ}\text{F}$. This choice is done by repeatedly pressing **READ** until the desired range is indicated.

Note: The temperature measurement unit ($^{\circ}\text{C}/^{\circ}\text{F}$) can only be changed after the device is activated in the menu. Learn more [Read and Change Settings](#) section.

Follow the Instruction for setting a positive temperature limit between $0^{\circ}\text{C}/0^{\circ}\text{F}$ and $+50^{\circ}\text{C}/+122^{\circ}\text{F}$ (internal sensor) or $0^{\circ}\text{C}/0^{\circ}\text{F}$ and $+55^{\circ}\text{C}/+131^{\circ}\text{F}$ (external sensor)

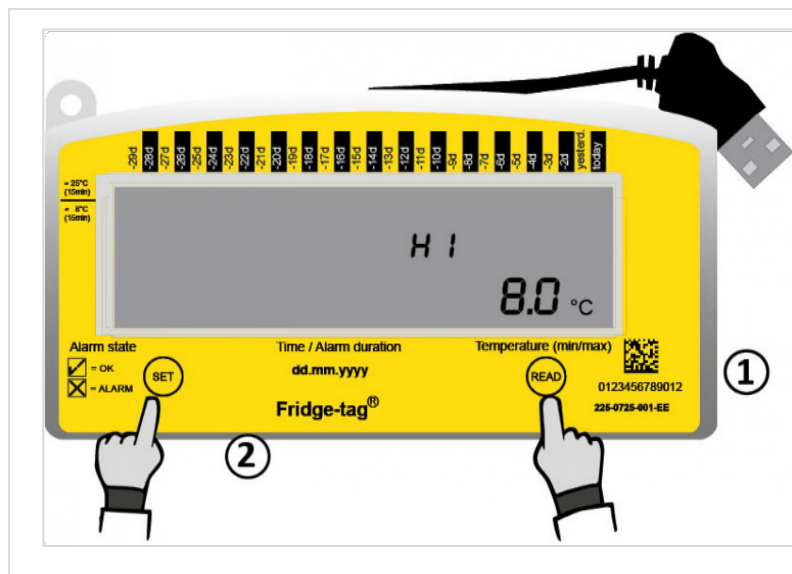


Press **READ** until the display shows no flashing sign.

Press **SET** to adjust the limit between 0°C/0°F and +50°C/+122°F.

The next digit can now be set. Press **READ** until you reach the desired number. Then press **SET** to confirm it. Then the next digit will start flashing. Continue until all digits of the alarm temperature are set.

Setting up a Fahrenheit Temperature Limit of +100°F or Higher


Note: The maximum Celsius temperature is +50°C (internal sensor) respectively +55°C (external sensor). This option is only available for temperatures in Fahrenheit.

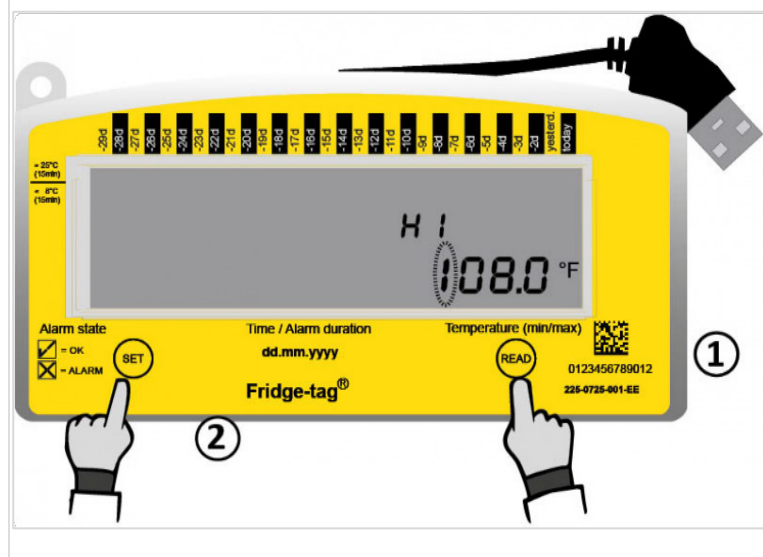

- Press **READ** until a leading "1" is flashing on the display.
- Press **SET** to adjust the limit equal or above +100°F.

The next digit of the temperature starts flashing. Continue until all digits of the alarm temperature limit are set.

Setting a negative temperature limit below 0°C/0°F

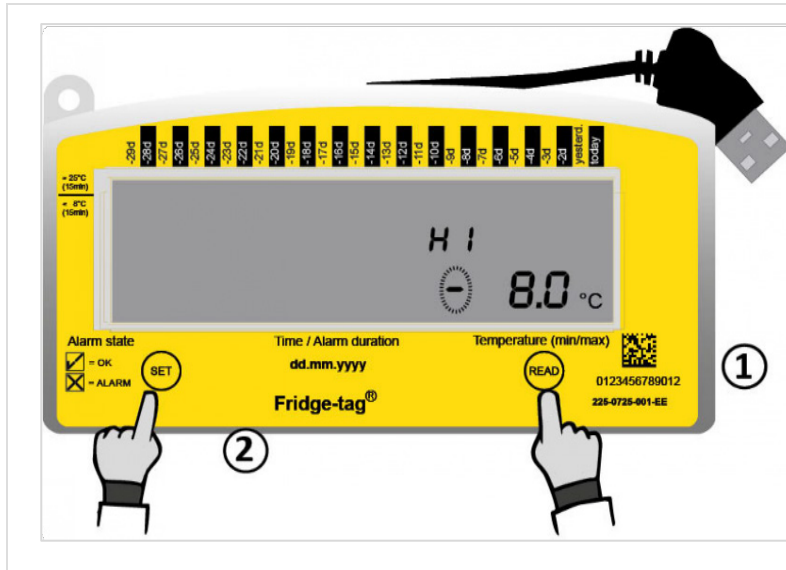

- Press **READ** until the “-” sign is flashing.
- Press **SET** to set the limit below 0°C/0°F.

1. Press **READ** until you reach the desired number.
2. Then press **SET** to confirm it. Then the next digit will start flashing.
3. Continue until all digits of the alarm temperature limits are set.

As soon as the parameters of the upper alarm limit are set, the first digit of the duration of the lower alarm limit will start flashing.

4. Proceed the same way as you did with the upper alarm limit.
- As soon as the last digit of the lower alarm limit is confirmed, the activation is completed.
 - **Internal sensor:** Now place the Fridge-tag according to [Placing the Fridge-Tag](#) section.
 - **External sensor:** Connect the device with the external sensor.

Note: In case the desired temperature limit cannot be confirmed, check if the temperature is set within the allowed operating temperature range.

LOC function (internal sensor only)

The Fridge-tag does not measure temperatures under the following circumstances:

- During the activation process of the device
- While pressing buttons (**READ** or **SET**)
- While the Fridge-tag is connected to a PC / Mac

After these actions have been completed, the Fridge-tag will not record temperatures for a period of 10 minutes (factory preset). In the display the symbol "LOC" displays. This function prevents false recordings of data which could be caused by heat while holding the device in the hands. Additionally, it allows an adaptation to the environmental temperature before normal recording continues.




- Even in LOC mode the user can press the **READ** button to retrieve historical information, change any setting or download a report to a computer. The whole LOC period will start again after the last button operation.
- If an action is interrupted, the device will start the LOC function approximately 30 seconds after last button operation.

Connection error (external sensor only)

After 10 minutes (factory preset) without a connection between the device and the external sensor **the whole display starts blinking**. Pressing **READ** will stop the display from blinking.

Display status: external sensor error

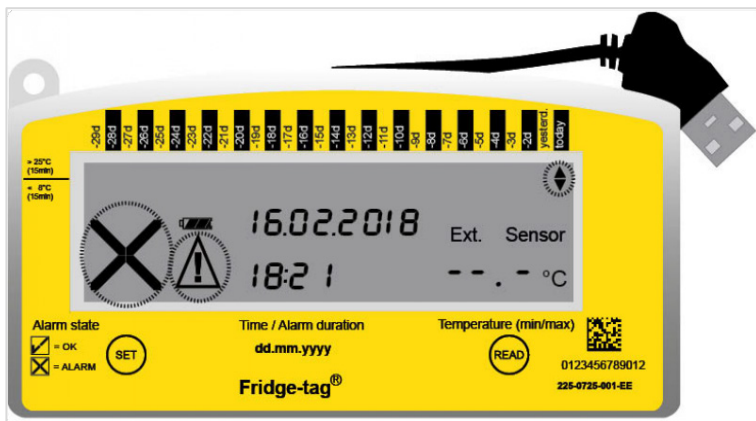


How to fix the connection error

Please check the following two points:

- Is the external sensors properly connected with the device?
- Does the external sensor cable have any defects?

Note: As soon as the error(s) have been cleared, the measuring will continue. During max. 1 minute after the connection no temperature is displayed on the screen.


Fix the connection error before stopping the warning. Otherwise, new temperature records will not be captured.

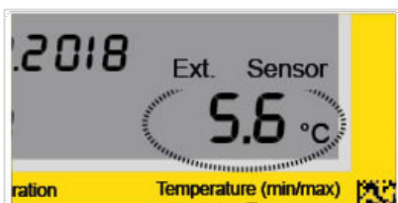

During a connection error no data will be recorded.

Read and Change Settings


Overview: menu

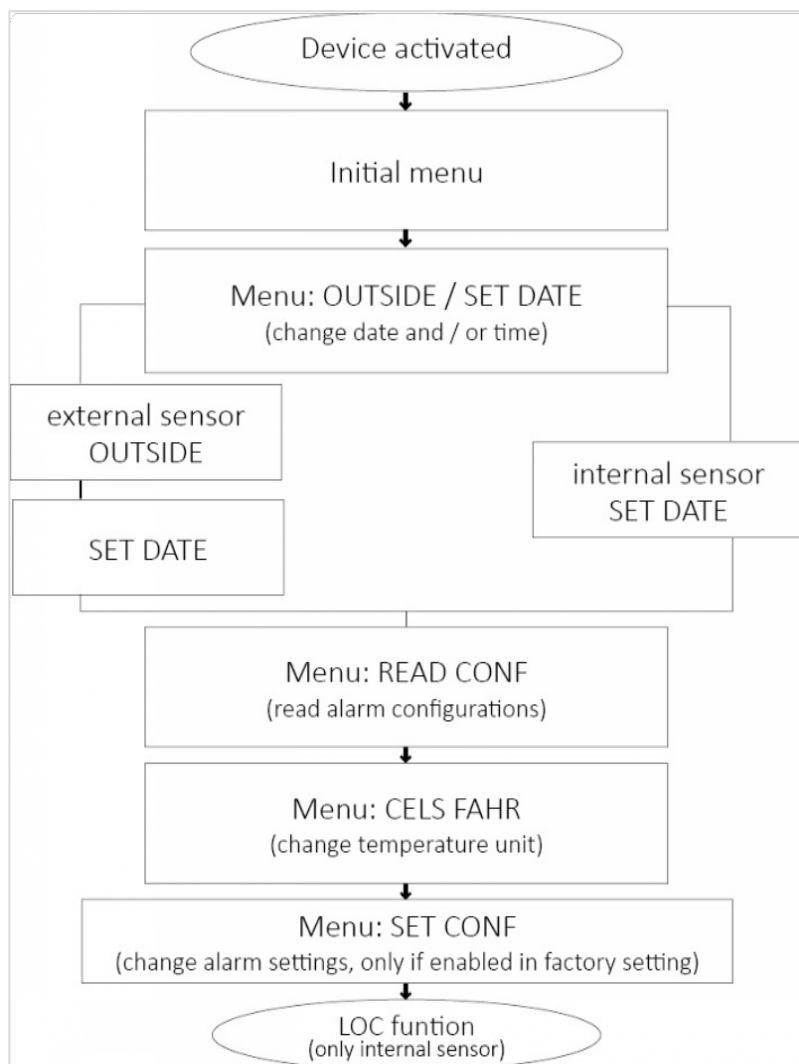

Note: If you scroll through the menu and you reach the LOC function (internal sensor) or the display of the measuring mode (external sensor) again you need to restart from the beginning by accessing the menu. In order to adjust more than one setting (e.g. time & Celsius to Fahrenheit) you must complete each change and return to menu mode for the 2nd change.

Initial menu (read and change settings)

To change the date format, the date, the time, the temperature measurement unit or the alarm settings or to read the preset alarm limits please proceed as follows:

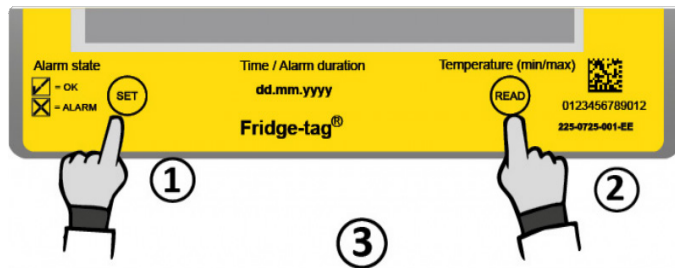

1. Press and hold **SET** ...
2. ... then press **READ** shortly ...
3. ... then release both buttons simultaneously.

- **SET DATE** (internal sensor) is now displayed on the screen.
- **OUTSIDE** (external sensor) is now displayed on the screen.

You entered the menu mode and may choose which entry to see or change.

- **OUTSIDE** (external sensor):
 - first screen shows the temperature measured with the internal sensor of the Fridge-tag (normal ambient temperature).
 - Press **READ** once to get to **SET DATE**.

Follow the instructions to access menus:

- **SET DATE** (internal sensor): Configuration with internal sensor,
- **SET DATE** is directly shown.
 - **SET DATE**: change date and/or time settings
 - **READ CONF**: read the alarm settings
 - **CELS FAHR**: change the temperature unit
 - **SET CONF**: change the alarm settings (only if enabled in factory setting)
- Use the **READ** button to scroll through the menu.
- Use the **SET** button to access the corresponding menu.

Access the menu "SET DATE"

- **External sensor**: The display shows **OUTSIDE**.
 - Press **READ** until the display shows **SET DATE**.
- **Internal sensor**: The display shows the menu **SET DATE**.
 - Press **SET** to access the menu to adjust the date format, date or time settings.
 - Follow the steps in the [Setting the Date](#) section.

Note: Changing the time or date does not affect alarm records. Users can update the date, time, or temperature unit as often as needed. Once activated, the device cannot be turned off. After any change, Fridge-tag locks for 24 hours from midnight after the modification for security (e.g., a change on September 15 triggers a lock from 00:01 am September 16 to 00:01 am September 17).

Access the menu “READ CONF”

The display shows **SET DATE** (internal sensor), **OUTSIDE** (external sensor).

- Press **READ** until the display shows **READ CONF**.
- Press **SET** to access the menu to read the current alarm configurations. First the display check appears.
- Press **READ** repeatedly to scroll through the preset alarm parameters.

Access the menu “CELS FAHR”

The display shows **SET DATE**.

- Press **READ** until the display shows **CELS FAHR**.
- Press **SET** to access the menu to change the temperature measurement unit.
- To change the measurement unit (Celsius/Fahrenheit) press **READ** until the display shows the desired sign (°C/°F).
- Press **SET** to confirm the measurement unit.

Access the “SET CONF” * Menu


The display shows **SET DATE**:

- Press **READ** until the display shows **SET CONF**.
- Press **SET** to access the menu to change the alarm configurations.
- To change the alarm limits (duration or temperature) please proceed as described in the [Setting the Alarm Limits \(if preset by factory\)](#) section.

*Changes of the alarm limits are only possible for devices which are programmed with this feature.


Screen Displays During Measurement Mode

Indication for max. 1 minute after completing the activation or after connecting the device with the external sensor. For a maximum of 1 minute no temperature is displayed on the screen, indicated by —.-

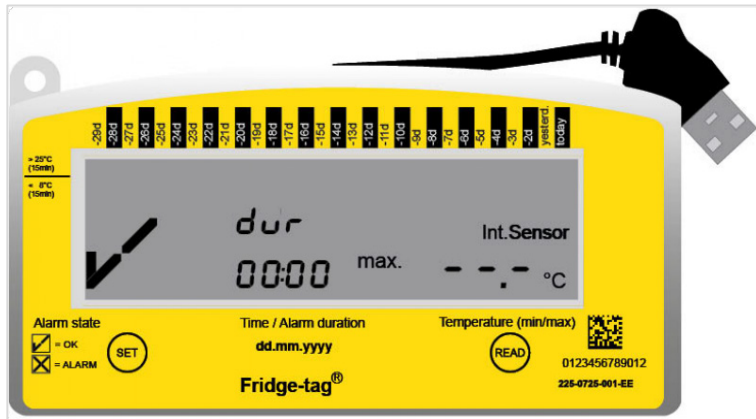


Example OK display – during measurement

- Once the device is fully activated the OK symbol ✓, the current temperature reading, the time and the date will be displayed on the screen.
- The Fridge-tag will also indicate whether the measuring is made with an internal sensor or an external sensor.
- The OK symbol ✓ is shown during normal operation as long as no alarms have been recorded. The temperature and time conditions were within the preset alarm limits.

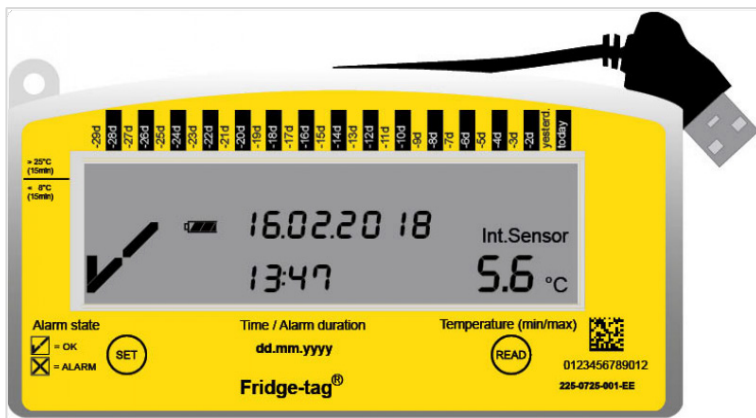

Example Alarm Display – During Measurement

If the preset alarm limits are exceeded, the following information will be displayed on the screen:

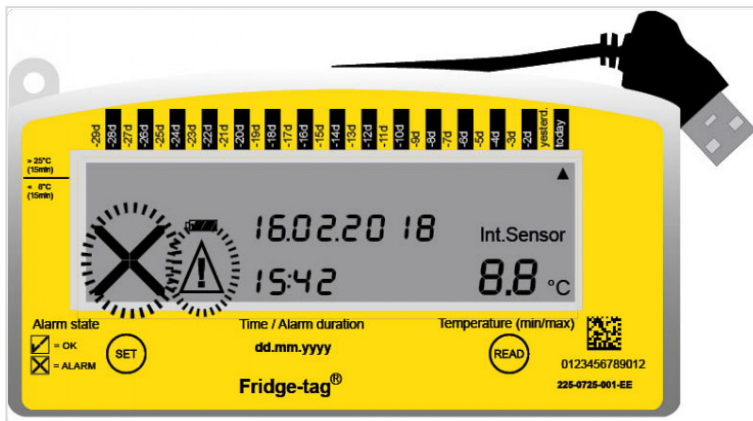

- ✓ (OK symbol) will be replaced by ✕ (alarm symbol)
- An additional alarm indicator ▲ will be indicated in the upper display area to show which alarm limit has been exceeded and on which day.
- In addition to the alarm symbol ✕ the warning symbol ⚠ will appear next to it.

Alarm Trigger Function

Single-event alarm triggering


The upper or lower alarm triggering is done with a single-event alarm algorithm. Any kind of alarm is triggered if the temperature is continuously out of the preset alarm limits for longer than the preset alarm trigger time.

Upper alarm triggering

Setting upper limit: Temperature $>8.0^{\circ}\text{C}$, duration >10 hours


For the upper alarm to be triggered the temperature needs to be continuously above 8°C for more than 10 hours.

Alarm triggered: alarm symbol ✕ and warning symbol ⚠ displayed.

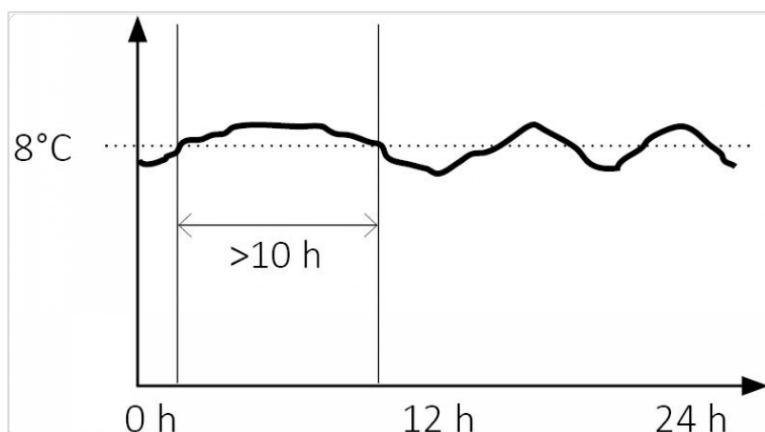

In the example below the sum* of the daily upper temperature deviation is about 20 hours. No alarm will be triggered! The temperature was not continuously out of the preset alarm limits for more than 10 hours in one row.

No Alarm triggered: OK symbol ✓ on the display.

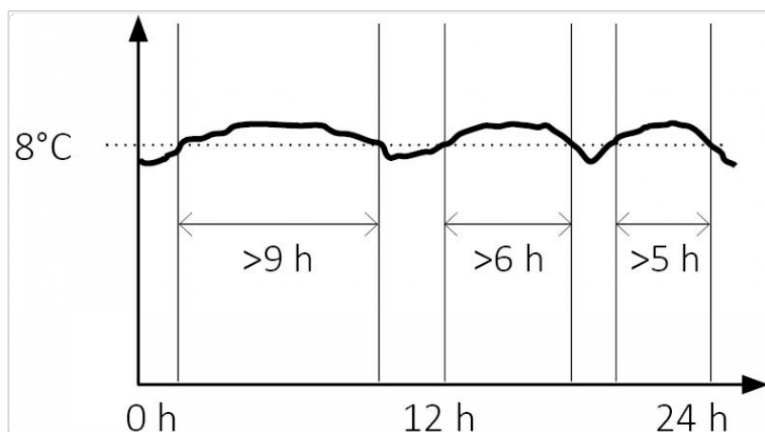


*The sum of the deviations is visible in the daily statistics in the column “Cumulative daily time above the limit.”

Lower alarm triggering

Setting lower limit: Temperature $< -0.5^{\circ}\text{C}$, duration > 1 hour


For a lower alarm to be triggered the temperature needs to be continuously below -0.5°C for more than 1 hour.

Alarm triggered: alarm symbol **✖** and warning symbol **⚠** displayed.

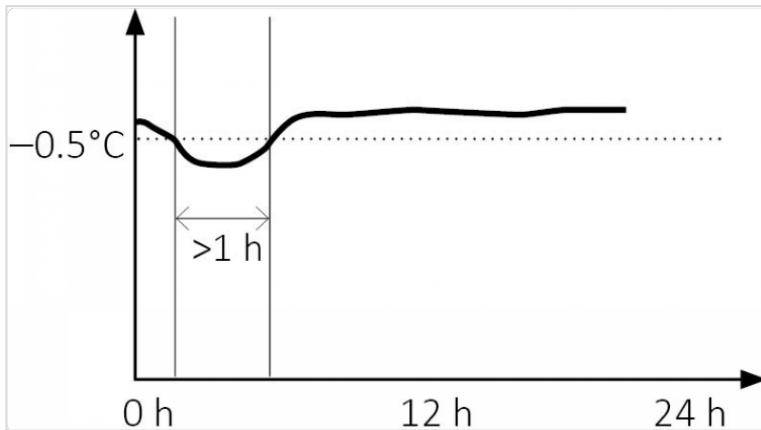

In the example below multiple low temperature deviations* are occurring. No alarm will be triggered. Each temperature deviation was less than 1 hour out of the preset alarm limits.

No Alarm triggered: OK symbol **✓** on the display.

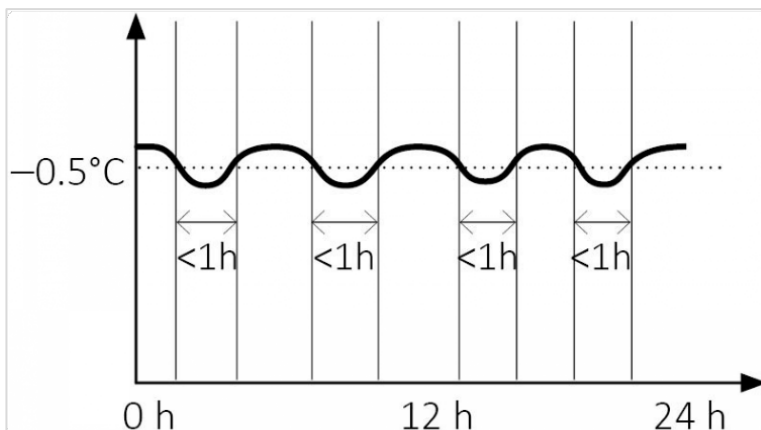


*The sum of the deviations is visible in the daily statistics in the column “Cumulative daily time below the limit.”


Alarm Display and Confirmation options

Option 1: Alarm indication “all alarms”

With this option, alarms will be visible on the display with an alarm symbol **✖** for 30 days:

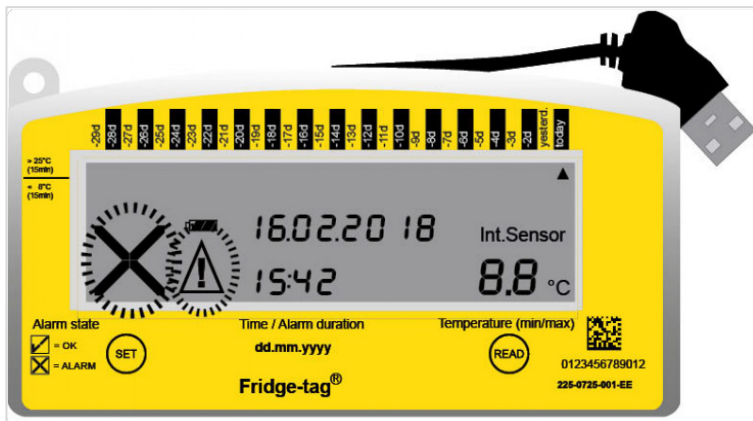

By pressing the **READ** button, the warning symbol Δ will be disabled for the corresponding alarms. The alarm symbol $\times$ cannot be canceled nor reset.

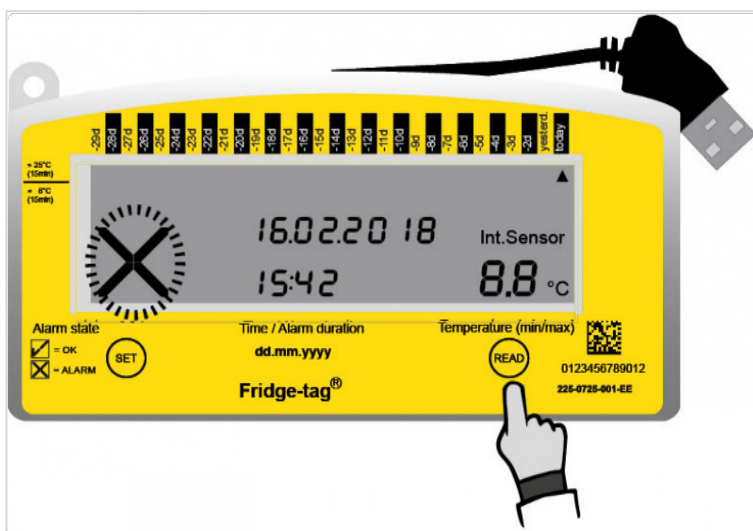


Note:


- In this mode only one upper and one lower alarm will be triggered per day.
- The alarm symbol $\times$ will be present on the display for 30 days.
- The warning symbol Δ can be deactivated by confirming all existing alarms in the readout mode.

Option 2: Alarm indication “unconfirmed alarms”

The alarms are shown with the alarm symbol $\times$ until all alarms (in the 30-day history) have been confirmed as solved by pressing the **READ** button. Afterwards the display will show the OK symbol $\checkmark$ until a new alarm is triggered.

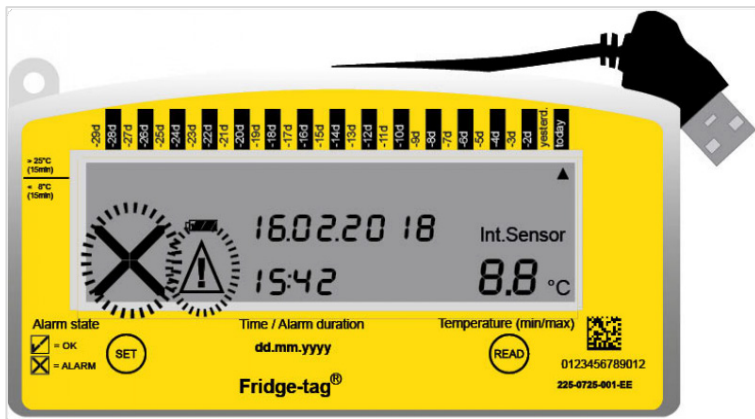

By pressing the **READ** button the warning symbol Δ will be disabled for the corresponding alarms. The alarm symbol $\times$ disappears and the OK symbol $\checkmark$ will be shown again.

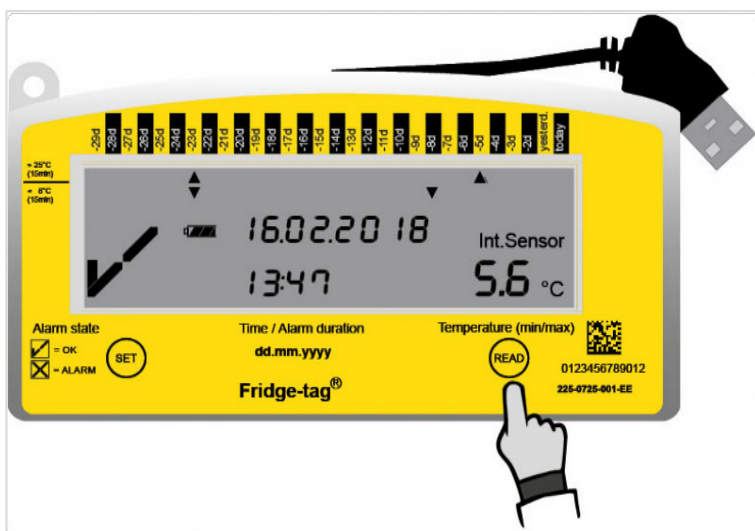


Confirmation Options of currently triggered alarms of the day

1. Device is within the set alarm limits

Press the **READ** button and the alarm symbol $\times$ and the warning symbol Δ will immediately disappear. A new alarm will be triggered as soon as the set alarm limits are exceeded again.

Settings: upper temperature limit $>8.0^{\circ}\text{C}$ and duration $>1\text{-hour}$, lower temperature limit $<-0.5^{\circ}\text{C}$ and duration 1 hour

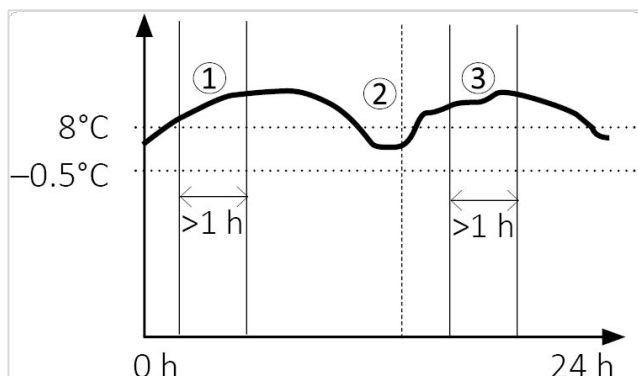


- Alarm triggered: alarm symbol ✕ and warning symbol ⚠ on display
- Alarm confirmed within the set temperature limits: OK symbol ✓ on display
- Alarm triggered: alarm symbol ✕ on warning symbol ⚠ on display.

2. Device is outside the set alarm limits

If the **READ** button is pressed still during a temperature violation the alarm symbol ✕ and the warning symbol ⚠ will stay on the display for the corresponding alarm.

Settings: upper temperature limit Temperature $>8.0^{\circ}\text{C}$ and duration $>1\text{-hour}$, lower temperature limit

$<-0.5^{\circ}\text{C}$ and duration 1 hour

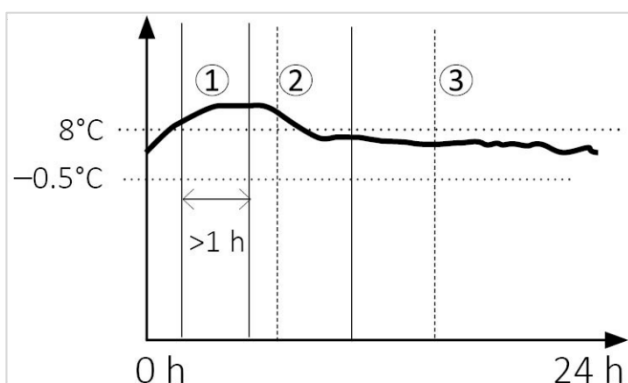

- Alarm triggered: alarm symbol ✕ and warning symbol ⚠ on display.
- Alarm confirmed when the temperature exceeds the set temperature limits: alarm symbol ✕ and warning symbol ⚠ remain on display.
- Temperature is back within the alarm limits. Now the alarm can be successfully confirmed. OK symbol ✓ on display.


Note: How the alarm symbol ✕ and the warning symbol ⚠ react is specified during configuration of the device in the factory settings.

Cumulative Daily Time Above/Below the Limit

The alarm trigger algorithm is based on a single event, although the Fridge-tag is measuring on a daily basis the individual total time above or below the temperature limits. This measurement is not used for any alarm condition. These recordings are only available in the generated PDF/ASCII files.

Note: It could be that the total cumulative time above/below the temperature limits is longer than the configured single-event alarm time without any alarm triggering.

Example setup: lower temperature limit $<-0.5^{\circ}\text{C}$, duration $>1\text{ hour}$

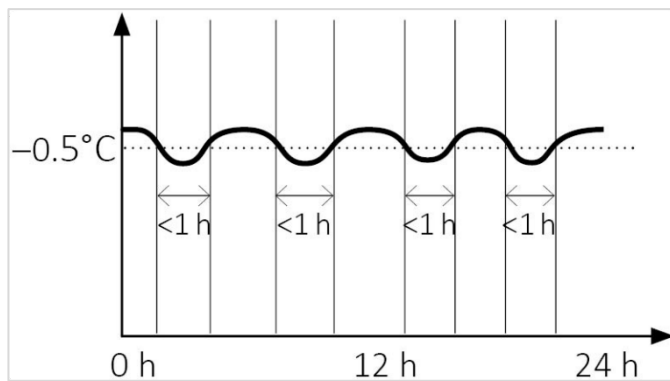

In the above example multiple low temperature deviations with exposure times of less than 1 hour occurred. The cumulative daily time below the limits adds up to about 3.5 hours but no alarm will be triggered. The same behavior also applies to the upper alarm.

Reading History / Readout Mode

The information of the temperature deviations can either be viewed for the past 30 days directly on the device or for 60 days in the generated files (PDF / ASCII).


Note: The external sensor of the Fridge-tag can remain at its location for the readout process. Please consider that a connection error may occur after more than 10 minutes without connection between the device and the sensor.

Option 1: Read From Device (30-Day History)

Example of an OK display during readout of the history

1. Press **READ** once


The following information is indicated on the screen:

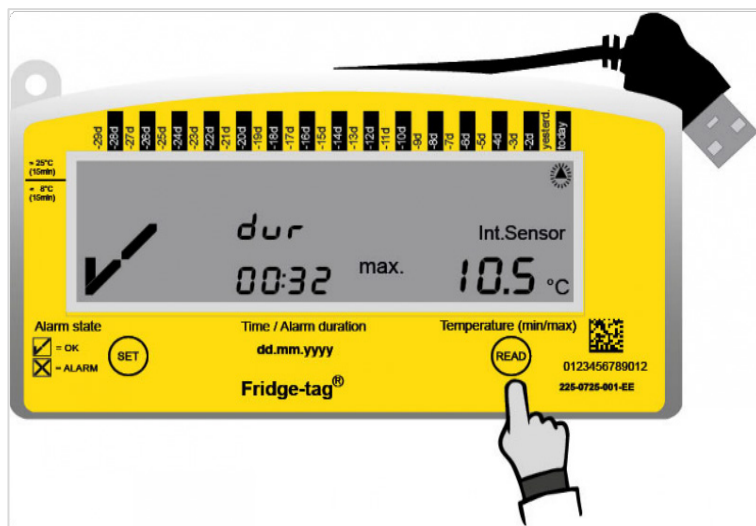

- The OK symbol ✓
- The corresponding flashing arrow ▲ (example: high arrow "today")
- Highest recorded temperature (example: +10.5°C)
- Duration of the exceedance of the preset high limit temperature (example 00:32; hh:min)

2. Press **READ** a second time

The following information is indicated on the screen:

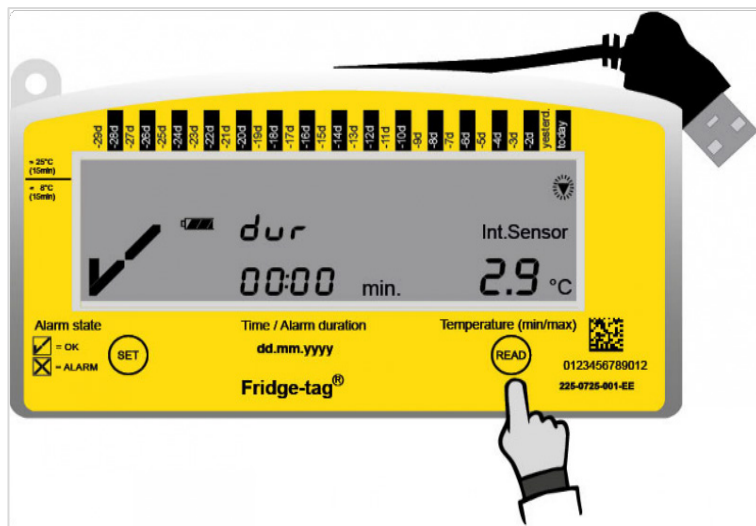

- The OK symbol ✓
- The corresponding flashing arrow ▼ (example: low arrow of “today”)
- Lowest recorded temperature (example: +2.9°C)
- Duration of the exceedance of the preset low temperature limit (example 00:00; hh:min)

Note: in the Readout mode the flashing arrows display the day where your are (30-day history) and show the highest ▲ and lowest ▼ measured temperature of the corresponding day. If a limit has been exceeded also the duration is shown.

Note: Press repeatedly the **READ** button to read out day per day the details of the past 30 days.


When you reach an alarm event, the indication on the screen of the Fridge-tag will be different than the OK display.

Example of an alarm display during readout of history

1st display of a “lower alarm event”

Press **READ** once

The following information is indicated on the screen:

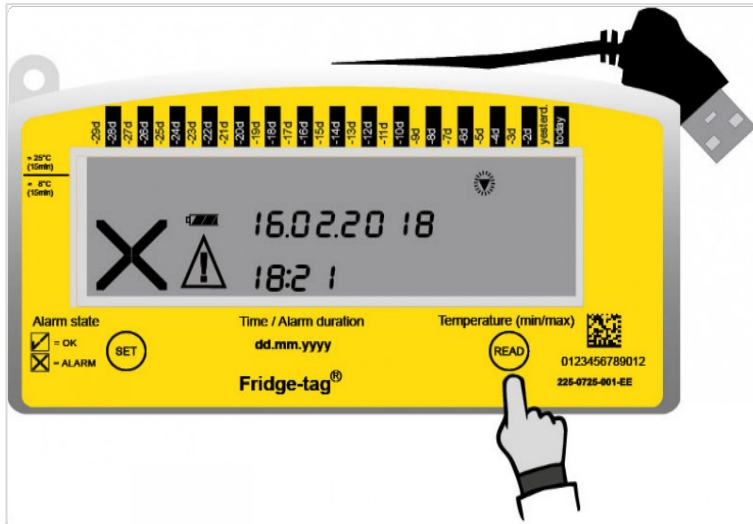


- The alarm- **X** and the warning symbol **!**
- The corresponding alarm indicator **▼** (lower alarm limit)
- Day of alarm (example: 5 days ago: -5d)
- The date of the alarm (example: 16.02.2018)
- The time of the alarm (example: 18:21)

2nd display of a “lower alarm event”

Press **READ** a second time

The following additional information is indicated on the screen:

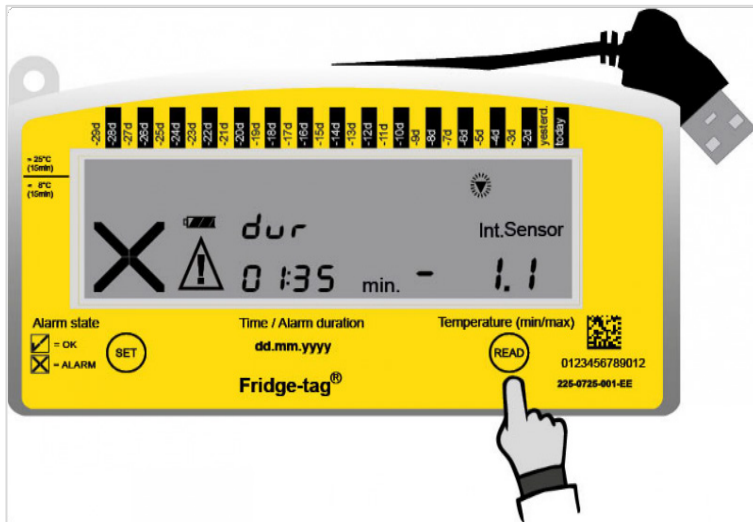

- Lowest recorded temperature (example: -1.1°C)
- The time elapsed until the preset low temperature threshold is exceeded (for example, 01:35; hh:mm).
- Temperature recording in this example with internal sensor


Option 2: Read Alarms on the Device (Alarm Super Jump Function)

Press the **READ** button for at least 3 seconds.

1st display of the latest alarm event

Press **READ** for 3 seconds

The following information is indicated on the screen:

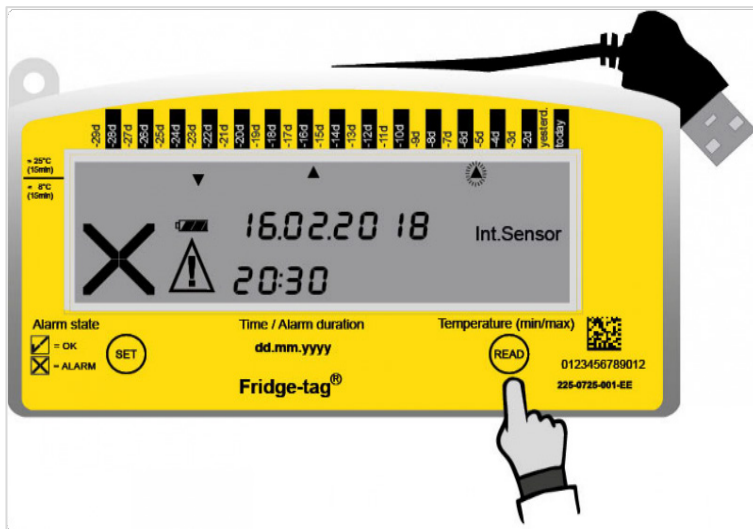


- The alarm symbol **X** and the warning symbol **⚠**
- The corresponding alarm indicator **▲** (higher alarm limit)
- Day of alarm (example: 5 days ago: -5d)
- The date of the alarm (example: 16.02.2018)
- The time of excursion (example: 20:30)

2nd display of the latest alarm event

Press **READ** again


The following additional information is indicated on the screen:

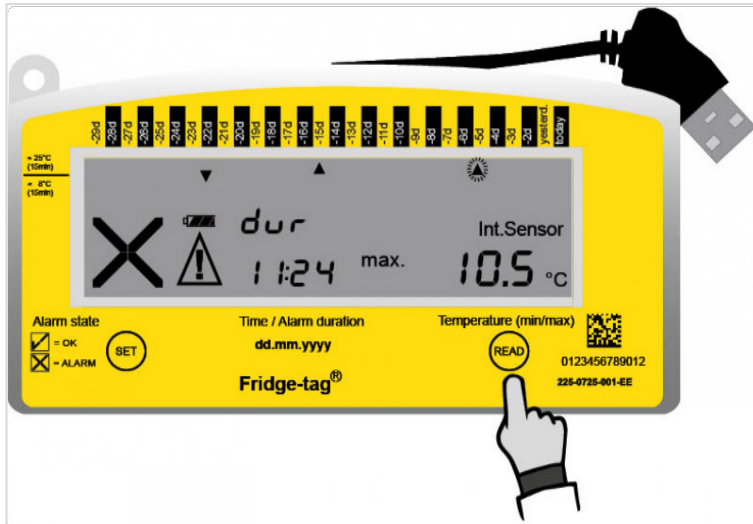

- Highest recorded temperature (example: +10.5°C)
- The duration of the exceedance of the preset high temperature limit (example: 11:24; hh:mm.)
- Temperature recording in this example with internal sensor

Note: Press the **READ** button again for at least 3 seconds and the next alarm event will appear on the screen.

Display of the next alarm event

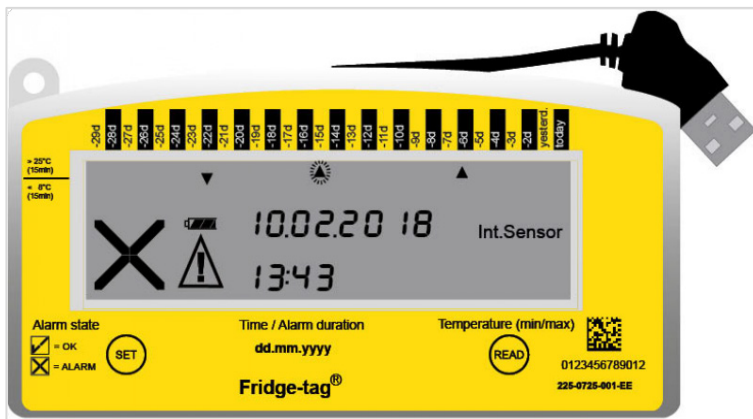


- Press the **READ** button again for 3 seconds to jump to the next alarm event. And so on.
- Pressing **SET** in the "Read out Mode" brings you back to the "Measurement Mode".

Option 3: Read Data from the Files Generated by the Fridge-Tag

Plug the Fridge-tag into any computer via USB interface. Make sure the device is plugged in properly.

Note: Disconnect the external sensor from the device first.

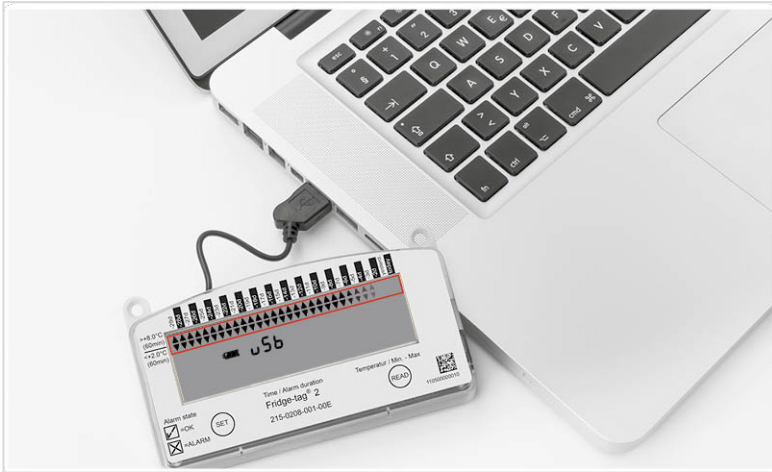


The Fridge-tag will now generate a PDF and ASCII report of the last 30, 60 days (factory preset). This process may take up to 30 seconds.


Choose the appropriate file generated by the Fridge-tag.

USB connection of the Fridge-tag


The continuously appearing arrows in the upper display area indicate that the device is processing.

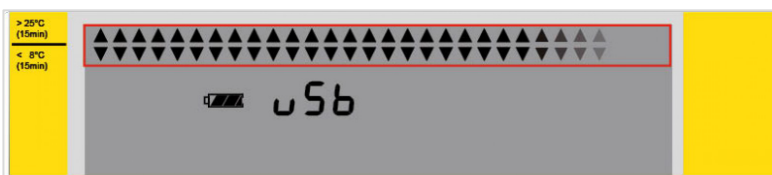


Note: This process must not be interrupted until the OK symbol  appears on the display. The example below indicates that the creation of the ASCII and PDF files as been successfully completed.

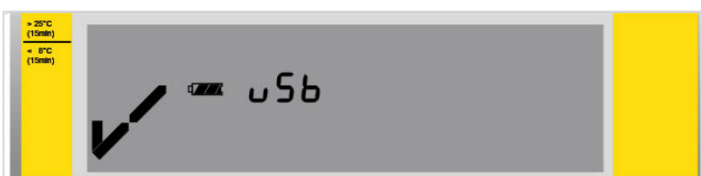

The device is shown in your explorer. Open the desired file generated by the device.

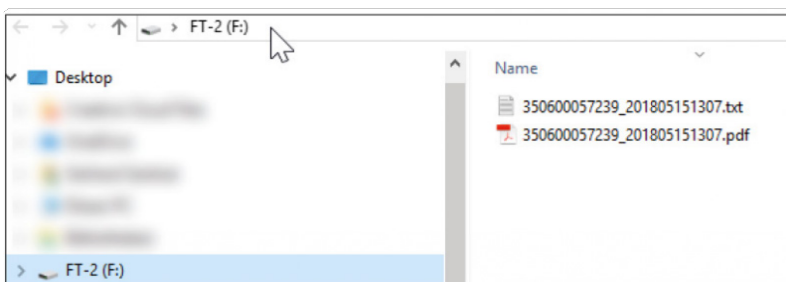

Note: To disconnect the device properly, please always use the function "Safely Remove Hardware" on your PC/Mac.

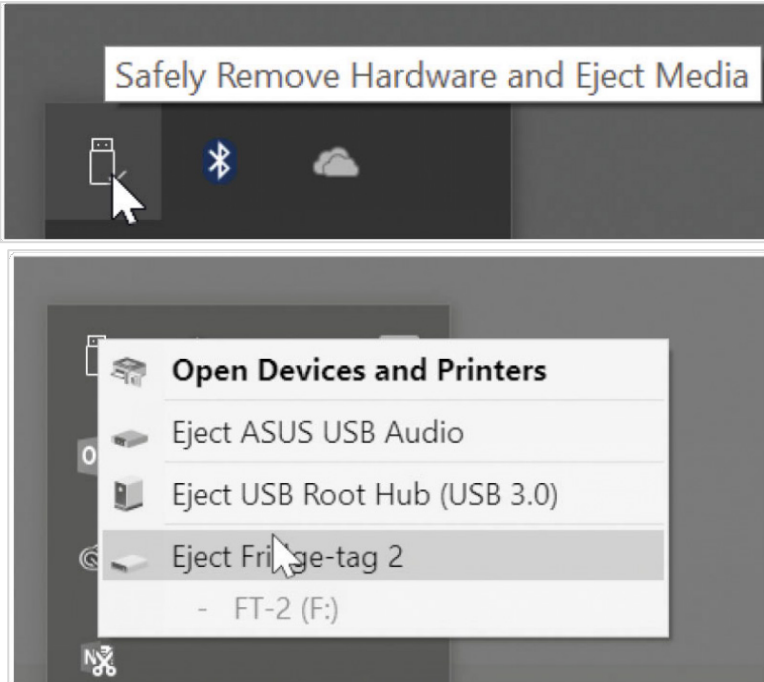	• Right-click the icon “Safely Remove Hardware and Eject Media” in the Windows taskbar (lower right corner). • Choose the corresponding device to remove.
	Do not disconnect the device before you receive the depicted message, otherwise the device can be damaged.

Note: For this process no additional software is necessary.

PDF Report Explanation

Sample of a PDF file generated by a Fridge-tag with external sensor

1 PDF document of the Fridge-tag

2 Identification number: 510500000006
 Date and time of report creation: 12/10/2017 20:37h
 Activation date: 01/05/2018 13:40h

3 Upper alarm limit: Above +8.0°C for 1min
 Lower alarm limit: Below +2.0°C for 1min

4 Measurement interval:¹⁾ 1min (fixed)
 Logging interval: 5min

5 Low battery since: 12/25/2017

6 Test String 1
 Test String 2
 Test String 3

7

No.	Date (MM/dd/yyyy)	Events ²⁾	Average temp.	Lower alarm limit				Upper alarm limit				Ext. sensor connection error			Signature / notes Action taken	
				Status	Min. temp.	Cumulative daily time below the limit	Alarm trigger time	Status	Max. temp.	Cumulative daily time above the limit	Alarm trigger time	Status	Duration	Alarm trigger time		
1	Today		+1.6°C	ALARM!	-1.0°C	11h 4min	00:00h	In progress	+5.9°C	0min			In progress	23h 59min	08:27h	
2	01/05/2018		+1.6°C	ALARM!	-0.9°C	17h 29min	00:00h	ok	+5.7°C	0min			ok	0min		
3	01/04/2018		+1.6°C	ALARM!	-1.0°C	16h 1min	00:26h	ok	+4.6°C	0min			ok	0min		
4	01/03/2018		+2.0°C	ALARM!	-0.7°C	16h 8min	00:00h	ok	+6.4°C	0min			ok	0min		
5	01/02/2018		+1.7°C	ALARM!	-1.4°C	14h 54min	00:00h	ok	+7.5°C	0min			ok	0min		
6	01/01/2018		+2.3°C	ALARM!	-0.7°C	9h 35min	06:19h	ok	+5.6°C	0min			ok	0min		
7	12/31/2017		+0.6°C	ALARM!	-5.3°C	9h 24min	00:00h	ok	+5.3°C	0min			ok	0min		
8	12/30/2017		-1.7°C	ALARM!	-5.1°C	22h 46min	00:01h	ok	+2.6°C	0min			ok	0min		
9	12/29/2017		+0.9°C	ALARM!	-4.2°C	13h 22min	00:00h	ALARM!	+8.6°C	14min	13:49h		ok	0min		
10	12/28/2017		-0.3°C	ALARM!	-3.4°C	20h 1min	00:00h	ok	+6.0°C	0min			ok	0min		
11	12/27/2017		+0.0°C	ALARM!	-2.9°C	19h 42min	00:00h	ok	+5.9°C	0min			ok	0min		
12	12/26/2017		+0.0°C	ALARM!	-2.2°C	16h 47min	00:00h	ok	+6.4°C	0min			ok	0min		
13	12/25/2017		+2.3°C	ALARM!	-0.5°C	13h 19min	02:28h	ALARM!	+8.3°C	24min	12:51h		ok	0min		
14	12/24/2017		+2.4°C	ALARM!	-1.2°C	11h 14min	00:00h	ALARM!	+8.6°C	30min	10:59h		ok	0min		
15	12/23/2017		+3.3°C	ALARM!	-1.3°C	10h 34min	00:00h	ALARM!	+11.0°C	2h 55min	12:05h		ok	0min		
16	12/22/2017		+3.3°C	ALARM!	-0.5°C	7h 25min	06:37h	ALARM!	+8.2°C	13min	12:53h		ok	0min		
17	12/21/2017	a 19:35	+5.0°C	ALARM!	+1.7°C	38min	22:41h	ALARM!	+8.3°C	32min	09:30h		ok	0min		
18	12/20/2017		+3.1°C	ALARM!	+0.3°C	10h 32min	00:00h	ALARM!	+10.2°C	2h 39min	11:27h		ok	0min		
19	12/19/2017		+4.0°C	ALARM!	+0.7°C	7h 33min	06:39h	ALARM!	+9.3°C	3h 4min	10:29h		ok	0min		
20	12/18/2017		+5.4°C	ALARM!	+0.4°C	4h 9min	00:00h	ALARM!	+10.8°C	4h 54min	10:03h		ok	0min		
21	12/17/2017		+4.6°C	ALARM!	+1.1°C	3h 18min	18:54h	ALARM!	+8.8°C	1h 38min	11:57h		ok	0min		
22	12/16/2017		+5.3°C	ALARM!	+1.9°C	3min	00:11h	ALARM!	+9.0°C	1h 14min	11:43h		ok	0min		
23	12/15/2017		+0.6°C	ALARM!	-2.6°C	14h 59min	00:00h	ok	+5.1°C	0min			ok	0min		
24	12/14/2017		-1.2°C	ALARM!	-4.1°C	20h 57min	00:01h	ok	+4.1°C	0min			ok	0min		
25	12/13/2017		-2.1°C	ALARM!	-5.7°C	21h 53min	00:00h	ok	+3.1°C	0min			ok	0min		
26	12/12/2017		+0.3°C	ALARM!	-4.5°C	16h 1min	00:00h	ok	+5.1°C	0min			ok	0min		
27	12/11/2017		-0.5°C	ALARM!	-1.7°C	5h 34min	18:27h	ok	+1.4°C	0min			ALARM!	18h 26min	00:00h	
28	12/10/2017		+26.6°C	ok	+25.3°C	0min		ALARM!	+27.6°C	2h 20min	13:42h		ALARM!	8h	16:16h	

8 1) Sampling and data analysis every minute
 2) 1 = time / date changed, a = alarm configuration changed, hh:mm = status checked

Date and place: _____ Signature: _____

9

- Document title and device type
- Device ID and self-explaining information
- Alarm settings
- Measuring and logging interval
- Event and alarm table (latest info in line 1, top line)
- Up to 3 user-definable strings (max. 30 characters each). Factory presetting
- Placeholder for notes
 - Note 1: Reference for measurement interval,
 - Note 2: Legend for events column (hh:mm → 1 time stamp/half day)
- Placeholder for date and signature
- Battery warning with timestamp

Temperature Record Duration (Optional Factory Setting)

Selectable record duration: 30, 60 days.

Note: File names on the Fridge-tag are write protected. The names may only be changed after downloading the files onto a computer. Changing is either possible directly on unopened files or via open and save commands with Adobe Reader. Using other programs may cause loss of the digital signature.

Date:	Date of measurement
Event: t	Time/date changed

Event: a	Alarm configuration changed
Event: hh:mm	Time stamp: status checked
Average temp.	Average temperature
Status: in progress	The data collection "Today" is not yet complete
Status: OK	No alarm has been triggered in the past 30 days. (No alarm has yet been triggered since the data was read out on the device. *)
Status: Alarm Δ	Alarm(s) have been triggered (With Δ means that the details of the corresponding alarm have not been read out yet. *)
Status: Alarm	Alarm(s) have been triggered (Without Δ means that the details of the corresponding alarm have already been read out on the device. *)
Min. temp.	Lowest recorded temperature
Cum. duration	Cumulative daily time below/above the limit
Alarm trigger time	Time at which the alarm was triggered
Max. temp.	Highest recorded temperature
Duration	Duration of an external sensor connection error

*For more information go to the [Alarm Trigger Function](#) section.

Verification process

This process verifies if the files (PDF and ASCII) created by the Fridge-tag are authentic and have not been manipulated or accidentally changed.

Note: Please ensure that the latest version of "JAVA Runtime" is previously installed on your computer.

1. Download the software Sensitech Verifier from our website: <https://sensitech.info/Verifier>
2. Open the software. The following window will appear:



3. Click **Open file**
4. Select the file you would like to verify.
 - a) Select the files directly from the Fridge-tag which is connected to your computer.
 - b) Select the files from the place where you saved them on your computer.

When the file is correct and in its original condition, the following window will appear:



In case the file has been changed, an error message will appear.



Proceed the same way with PDF and ASCII files. The same OK or error messages will appear.

Explanations of terms

Readout mode

In order to avoid incorrect data, the Fridge-tag does not measure the temperature while settings are changed or during Readout mode (e.g. changing time, date and during reading of history). The Fridge-tag will fall back into normal operation after approx. 60 seconds without pressing any buttons. The LOC function will be activated (internal sensor).

External sensor

After 10 minutes (factory preset) without connection between external sensor and device the entire display starts flashing.

HI or LO indicator

If the Fridge-tag measures temperatures above +55°C or below –40°C, it shows HI or LO on the screen. The regular measurements and monitoring of alarm limits will continue as usual. As soon as the temperature is between +55°C and –40°C numbers will be displayed again.

Expire code explanation

Learn more about your Fridge-tag  www.berlinger.com/support/fridge-tag	Production date
	Quality control passed
	Expiry date (Estimated battery-life-time)
Date of activation / location	

Production Date:	Feb., 2019 (example)
Quality control:	Passed
Expiry Date:	Aug., 2022 (example) estimated Battery-life-time
Date of activation:	Write the date of activation in this field.

Important Information

Liability

The manufacturer shall not be held liable:

- If the device was used beyond the manufacturer's given limitations.
- For any claims due to the improper storage or use of the device.
- For any problems with the temperature-controlling and/or -cooling unit.
- For the quality of any monitored goods.
- For incorrect readings if the device was used beyond its expiry date.

Warranty: 2 years from date of delivery.

Battery

The Fridge-tag contains a CR Lithium battery. Please pay strict attention to the following points:

- The housing of the Fridge-tag must never be opened nor destroyed.
- Never expose the Fridge-tag to high temperatures (fire, oven, microwaves, etc.). It may cause injuries.
- Always keep the Fridge-tag out of the reach of children.
- The battery complies with IATA DGR Packing Instruction 970-Section II and is therefore not considered as dangerous good.
- Dispose or recycle the Fridge-tag in accordance with the WEEE 2012/19/EU guidelines or your local regulations. The device may also be returned to the manufacturer for proper recycling.

Useful life

The Fridge-tag 2 can be used up to 3 1/2 years after production date (1/2 year storage / 3 years useful life), the Fridge-tag 2 E can be used up to 5 1/2 years after production date (1/2 year storage / 5 years useful life), on the condition that:

- The buttons are not pressed for very long time.

Note: Avoid jamming the device between the goods to be monitored in a shipment.


Storage and operation of the device remains inside the recommendations of the manufacturer. Especially temperatures below 0°C or +32°F could have a negative influence on the operating lifetime of the battery.

The end of the lifetime of the battery is indicated by the battery indicator on the display (see Display Explanations section).

Attention

The Fridge-tag measures the ambient temperature and not the quality of the monitored goods. Its purpose is to signal if product quality evaluation is required.

Regulatory certification

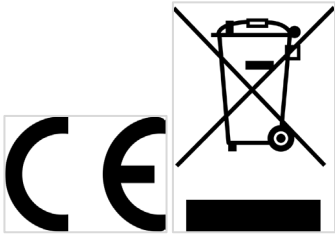

FAQ / Glossary

Frequently Asked Questions (FAQ)

For technical problems or questions, please visit the Sensitech Support Center: Fridge-tag 2x Family.

Glossary of Symbols

Symbol	Description
	OK symbol
	alarm symbol
	LOW alarm indicator
	HIGH alarm indicator
	warning symbol

The warning box includes important information or warnings.